



## **Mathematical modelling of intraoperative gas exchange in extracorporeal oxygenation**

Downloaded from: <https://research.chalmers.se>, 2026-10-18 02:21 UTC

Citation for the original published paper (version of record):

Schulte, D., Scampicchio, A., Schmid Daners, M. et al (2026). Mathematical modelling of intraoperative gas exchange in extracorporeal oxygenation. Proceedings on Automation in Medical Engineering, 3(1). <http://dx.doi.org/10.18416/AUTOMED.2026.2480>

N.B. When citing this work, cite the original published paper.

# Mathematical modelling of intraoperative gas exchange in extracorporeal oxygenation

D. T. Schulte<sup>1\*</sup>, A. Scampicchio<sup>1,2</sup>, M. Schmid Daners<sup>1</sup> and M. N. Zeilinger<sup>1</sup>

<sup>1</sup> Intelligent Control Systems, ETH Zurich, Zurich, Switzerland

<sup>2</sup> Department of Electrical Engineering, Chalmers University of Technology, Göteborg, Sweden

\* Corresponding author, email: schulted@ethz.ch

*Abstract: During cardiopulmonary bypass surgery, a key role is played by the oxygen and carbon-dioxide exchange between the body and the oxygenator. In this work, we present a preliminary mathematical model of this gas exchange and show some results based on experimental data in piglets.*

© 2026 Dominik Thomas Schulte; licensee Infinite Science Publishing

This is an Open Access article distributed under the terms of the Creative Commons Attribution License CC-BY 4.0., which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

## I. Introduction

Several studies have indicated that cardiopulmonary bypass (CPB) during surgical correction of congenital heart defects may contribute to white matter injuries in neonates [1,2]. The underlying mechanisms responsible for these injuries remain poorly understood, largely because MR imaging cannot be performed intraoperatively, since conventional CPB systems are not safe for use near an MR scanner. In previous work, we addressed this limitation by developing an MR-conditional heart-lung machine (HLM) that enables MR imaging during CPB procedures [3,4]. Using this system, we conducted in-vivo experiments on piglets to obtain preliminary data [5]. However, the available dataset is not sufficient to fully explain the causes of the observed neurological damage. To overcome this issue, we aim at creating a full data-informed model of the relevant physiological processes. As a first step towards this goal, in this work we focus on the oxygen (O<sub>2</sub>) and carbon dioxide (CO<sub>2</sub>) exchange within the oxygenator of the MR-conditional HLM. Specifically, we build upon the mathematical model introduced by [6], which describes the O<sub>2</sub> and CO<sub>2</sub> exchange within a hollow fiber membrane oxygenator, and estimate the O<sub>2</sub> and CO<sub>2</sub> contents and partial pressures on the venous side using the initial values on the arterial side and the HLM settings.

## II. Material and methods

We start by considering Eqs. (9) and (12) of [6] yielding the O<sub>2</sub> transfer rate (OTR) and CO<sub>2</sub> transfer rate (CTR):

$$OTR = \dot{Q}_B (CaO_2 - CvO_2) \quad (1)$$

$$CTR = \dot{Q}_B (CvCO_2 - CaCO_2) \quad (2)$$

where  $\dot{Q}_B$  (L/min) is the blood flow rate, and  $CxO_2$  and  $CxCO_2$  (mL/L blood) are the O<sub>2</sub> and CO<sub>2</sub> contents on the arterial and venous sides if  $x = a$ , and  $x = v$ , respectively. Next, we note by Fick's law [7] that

$$CvO_2 = CaO_2 - \frac{\dot{V}O_2}{\dot{Q}_B} \quad (3)$$

$$CvCO_2 = CaCO_2 + \frac{\dot{V}CO_2}{\dot{Q}_B} \quad (4)$$

where  $\dot{V}O_2$  and  $\dot{V}CO_2$  (mL/min) are the O<sub>2</sub> consumption and CO<sub>2</sub> production, which can be calculated starting from body weight ( $BW$ , which is around 15 kg for piglets) and temperature  $T$  (°C) from [7] and [8]:

$$\dot{V}O_2 = 32.394 \cdot BW^{0.375} \cdot 4 \cdot 10^{-7} \cdot T^{4.077} \quad (5)$$

$$\dot{V}CO_2 = 5.9319 \cdot BW^{0.75} \cdot 4 \cdot 10^{-7} \cdot T^{4.077} \quad (6)$$

By combining (3) with (5) and (4) with (6), we obtain that  $OTR = \dot{V}O_2$  and  $CTR = \dot{V}CO_2$ . We can now derive the unknown partial pressures on the venous side,  $PvO_2$  and  $PvCO_2$  (mmHg). At the start of the operation, we measure the partial pressures on the arterial sides, namely  $PaO_2$  and  $PaCO_2$  for O<sub>2</sub> and CO<sub>2</sub>, respectively. The values for the venous side,  $PvO_2$  and  $PvCO_2$ , are computed from (3), (4) using mathematical models for O<sub>2</sub> and CO<sub>2</sub> contents ([6] Eqs. (4), (7)) as follows. By using  $x \in \{a, v\}$  for either arterial or venous side, we have:

$$CxO_2 = 10(1.34 \cdot tHb \cdot SxO_2 + PxO_2 \cdot \alpha_{O_2} \cdot \left(1 - \frac{Hct}{100}\right)) \quad (7)$$

$$CxCO_2 = 22.6 \cdot \alpha_{CO_2} \cdot PxC O_2 \cdot 10^{pH_x - pK} \cdot \left(1 - \frac{0.0289 \cdot tHb}{(3.352 - 0.0046 \cdot SxO_2)(8.142 - pH_x)}\right) \quad (8)$$

where  $Hct$  (%) and  $tHb$  (g/dL) are the measured hematocrit and the hemoglobin content, respectively, and  $pK = 6.0907$  is the apparent dissociation coefficient of the  $CO_2/HCO_3^-$  system. The solubility coefficients  $\alpha_{O_2}$  (mL O<sub>2</sub>/dL blood/mmHg) and  $\alpha_{CO_2}$  (mmol CO<sub>2</sub>/L blood/mmHg), oxygen saturation  $SxO_2$  and  $pH$  are computed from the partial pressures as follows [6,9]:

$$\alpha_{O_2} = 0.1358(0.0276 \cdot e^{-0.0361T} + 0.0143) \quad (9)$$

$$\alpha_{CO_2} = 0.05874(0.9454 \cdot e^{-0.0625T} + 0.6539 \cdot e^{-0.012T}) \quad (10)$$

$$SxO_2 = \frac{PxO_2^{2.9}}{PxO_2^{2.9} + PxO_{2,50}^{2.9}} \quad (11)$$

$$PxO_{2,50} = 32.558 \cdot 10^{(-0.266(\ln(40) - \ln(PxCO_2)))} \quad (12)$$

$$pH_x = 6.1 + \log_{10} \left( \frac{PxCO_2 - 16.08}{0.03 \cdot PxCO_2} \right) \quad (13)$$

where the last relation implies that  $[HCO_3^-] = PxCO_2 - 16.08$  derived from experimental data.

Ultimately,  $PvO_2$  and  $PvCO_2$  are obtained from solving (3) and (4) substituting (7) – (13). The two nonlinear equations are solved in MATLAB setting the constraints  $5 < PvO_2 < 200$  mmHg and  $10 < PvCO_2 < 100$  mmHg (to ensure numerically stable and clinically plausible estimates under surgical conditions [10]) using the interior-point method implemented by “fmincon”.

### III. Results and discussion

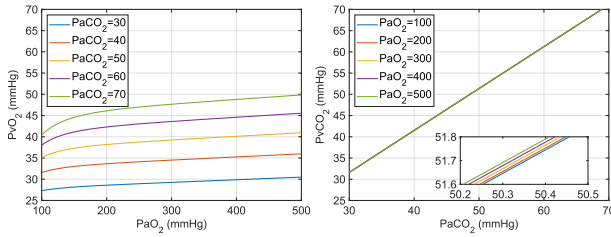


Figure 1: Predicted behavior of simulated venous partial pressures against arterial ones, oxygen part (left) and carbon dioxide part (right). We set  $T=35$  °C,  $tHb=10.3$  g/dL,  $Hct=30.9\%$ ,  $BW=15$  kg,  $\dot{Q}_B = 800$  mL/min,  $\dot{Q}_G = 1000$  mL/min.

We start by plotting a sample behavior of our model on synthetic data in Figure 1. We depict the value of  $PvO_2$  as a function of  $PaO_2$  for different values of  $PaCO_2$  on the left; similarly, on the right we focus on  $PvCO_2$  as a function of  $PaCO_2$ . All other parameters are not changing. We can notice that the carbon dioxide side displays a linear behavior quite consistent across  $PaO_2$  values, while linearity on the oxygen part emerges only after approximately  $PaO_2 = 200$  mmHg, and the values of  $PaCO_2$  have a notable impact.

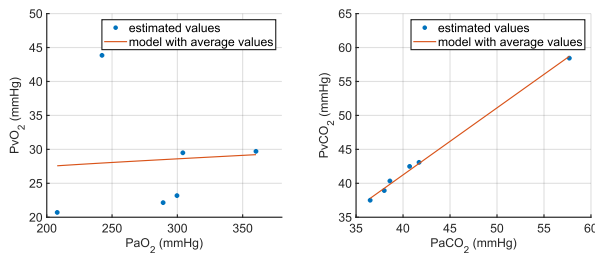


Figure 2: Estimated venous partial pressures for oxygen (left) and carbon dioxide (right) obtained from in-vivo data. The line represents the model output, obtained similarly to Figure 1, but setting the other parameters equal to the observed means throughout the experiment.

This impact is also reflected in the test on experimental data reported in Figure 2. The partial pressures of  $O_2$  and  $CO_2$  that are measured during one of the experiments are depicted. We compare the measurements, reported as dots, against the output obtained from our model, where  $T$ ,  $tHb$ ,  $Hct$ ,  $\dot{Q}_B$  and  $\dot{Q}_G$  are set to the mean values observed throughout the experiment. We can see the substantial

impact of the other parameters in the  $PaO_2 - PvO_2$  model (Figure 2, left panel); in contrast, for  $CO_2$  (Figure 2, right panel) the model captures the behavior of the data even if the values of  $T$ ,  $tHb$ ,  $Hct$ ,  $\dot{Q}_B$  and  $\dot{Q}_G$  are set to their average. It can be noticed that  $PaCO_2$  is maintained close to the intended range for the in-vivo study, while  $PaO_2$  is increased above physiological levels in accordance with standard clinical practice [10]. The venous partial pressures  $O_2$  and  $CO_2$  fall within physiological ranges for both  $PvCO_2$  (24.2 – 48.2 mmHg) and  $PvO_2$  (24.79 – 114.17 mmHg) [11].

The main limitation of this study is the small amount of data available. With additional measurements, the model could be improved by fitting the equations shown directly to the experimental observations. Furthermore, the calculated venous partial pressures could not be validated against measured results, as no venous blood gas analysis was performed during the experiments, but the results appear physiologically consistent.

### IV. Conclusions

The proposed modeling approach for estimating venous partial pressures of blood gases demonstrates promising results. The estimated values fall within physiological ranges and show good agreement with experimental data. By enabling estimation of venous partial pressures, the model also allows for the calculation of the updated arterial partial pressures, creating a comprehensive framework to predict dynamic changes in blood gas partial pressures over time.

#### AUTHOR’S STATEMENT

Research funding: Innosuisse – Swiss Agency for Innovation Promotion (56642.1 IP-LS) and the Wallenberg AI, Autonomous Systems and Software Program (WASP) funded by the Knut and Alice Wallenberg Foundation. Conflict of interest: Authors state no conflict of interest.

#### REFERENCES

- [1] Beca J, *New White matter brain injury after infant heart surgery is associated with diagnostic group and the use of circulatory arrest*, Circulation, Vol. 127, pp. 971–979, 2013
- [2] Andropoulos DB, *Brain immaturity is associated with brain injury before and after neonatal cardiac surgery with high-flow bypass and cerebral oxygenation monitoring*, Journal of Thoracic and Cardiovascular Surgery, Vol. 139, pp. 543–556, 2010
- [3] Schulte DT, *Hydraulic in-vitro Characterization of MR-conditional Blood Pumps*, Artificial Organs, 2025
- [4] Schulte DT, *Preliminary In-vitro Hemolysis Evaluation of MR-conditional Blood Pumps*, Frontier in Medical Technologies, 2025
- [5] Schulte DT, *Cerebral hemodynamic changes during cardiac surgery: a feasibility MR study in piglets*, NMR in Biomedicine (under consideration).
- [6] Khadka LB, *Mathematical Modeling of Oxygen and Carbon Dioxide Exchange in Hollow Fiber Oxygenators*, in Up-to-Date Approach to Blood Gas Analysis - Clues to Diagnosis and Treatment, London, Ozgur Karcioglu, Ed. IntechOpen, 2024
- [7] Higuchi H, *Whole-body oxygen consumption at different temperatures during cardiopulmonary bypass*, Kyobu Geka, Vol. 53, pp. 841–846, 2020
- [8] Rodriguez MR, *Evolution and Neural Network Prediction of CO2 Emissions in Weaned Piglet Farms*, Sensors Vol. 22, pp. 2910, 2022
- [9] Christmas KM, *Equations for O2 and CO2 solubilities in saline and plasma: combining temperature and density dependences*, J Appl Physiol, Vol. 122, pp. 1313, 2017
- [10] Fontes MT, *Arterial Hyperoxia During Cardiopulmonary Bypass and Postoperative Cognitive Dysfunction*, J Cardiothorac Vasc Anesth, Vol. 28, pp. 462–466, 2014
- [11] Lee S, *Analysis of blood composition by porcine breeding cycle*, Vet Med Sci, Vol. 10, e31376, 2024